

rebound
GLOBAL TRADING CO.



 **powerbone**[®]
pioneer of health



Website

CE 01.26/REV10/22.07.2022

BONEGRAFT[®]
— BIOMATERIALS —



INDEX

4	About Powerbone
5	Mission and Vision
6-7	Pioneer of R&D
8-9	Powerbone Production Technology
10-29	Powerbone Production Standards
30-41	Product References and Values



POWERBONE

A biotechnology company that focuses on the development, manufacturing and marketing of innovative and functional biomaterials.

Powerbone Biomaterials Co. is one of the leading company in the world that can produce osteoinductive and osteoconductive synthetic bone graft materials, barrier membrane, bone cement and cartilage graft.

Powerbone R&D activities take place at Ege University Technology Development Centre under ISO-7 (Class 10000). Since 2016 production to ISO-5, ISO 6 and ISO-7 (Class 100,1000,10,000) conditions takes place in Manisa.

In addition to expert employees, high technology and strong capital, Powerbone Biomaterials customer service exceeds Internationally recognised quality and management standards.



R&D-Oriented Production



Production

Powerbone's modern production facility is electronically controlled. Multiple production parameters are observed in real time 24/7 according to ISO7 standard. The production areas are monitored according to ISO14644 Class 10.000 and Fed.Std.209 D, ISO5. ISO 14644 is applied to the clean rooms and packaging areas to Fed.Std.209D

All raw materials and equipment used in production processes are supplied from European and American companies with the highest technological standards.

TSE approved TS EN ISO 13485 Quality Management System

Our products bear the CE mark as Class III Medical Device, in which the highest level of safety standards are applied to the production conditions. Product quality control tests are carried out in reputable universities and test organizations in Turkey and abroad.

Quality


Quality control is carried out in accordance with production instructions using measurement devices unique to each specific medical device.

BIOMATERIAL INNOVATION REPLACED BY NEW BONE

- Innovative Flexible Bone Graft
- Connected high pore structure, cross-section of bone grafts for different geometries and sizes
- Bone graft in injectable form that does not require mixing


R&D

Our R&D unit, located in Ege University Technology Development Zone has a special focus on novel synthetic technologies designed for tissue engineering and regeneration of bone and cartilage tissue.

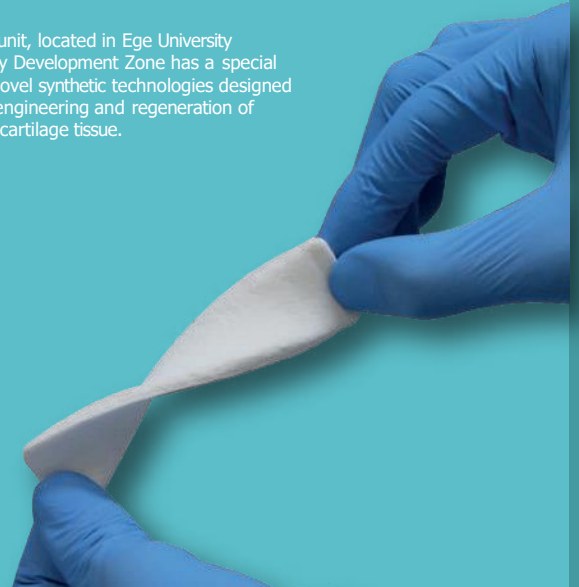

POWERBONE PRODUCT TECHNOLOGY

Powerbone Biomaterials are designed to repair bone defects caused by surgery or traumatic injury, to increase bone formation or support the formation of new bone tissue in non-load bearing sites. Many of our biomaterials can be mixed with bone marrow, blood products, pharmaceuticals such as antibiotics or other bone grafts materials.

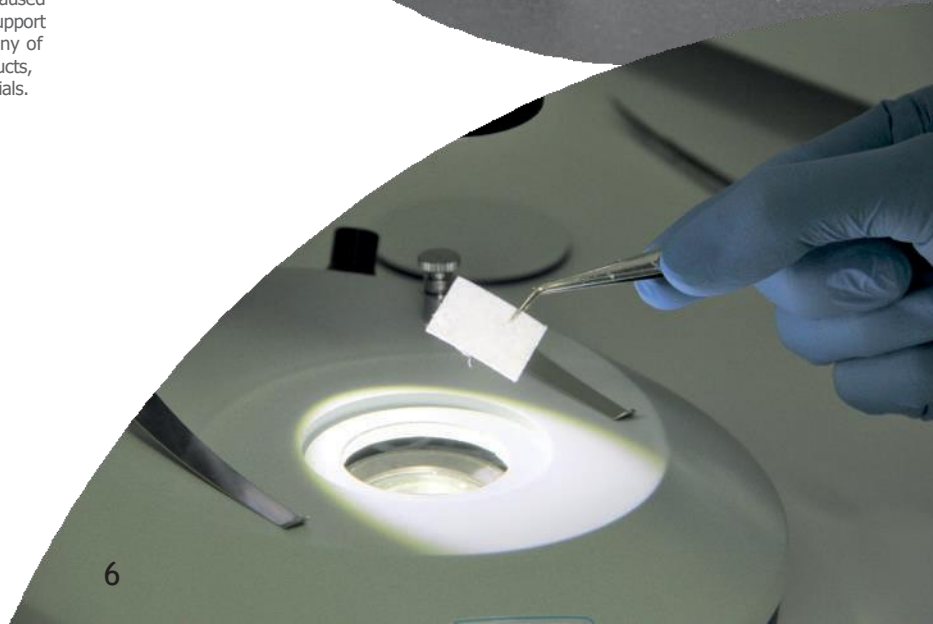

CERTIFICATES



CE



- ISO - 13485
- ISO 9001
- CE Certificates for each product groups



PRODUCTS

SILICATE ADDITIVE GRANULE, STICK & BLOCK

- Osteoconductive and Osteoinductive
- The high porosity of Powerbone products support initial clot stabilisation.
- Calcium phosphate provides a conductive scaffold for blood vessels and bone stimulating cells - a structure very similar to the mineral component of natural bone.
- Powerbone materials include silicate which increases circulating protein retention giving bioactive characteristics to the graft.

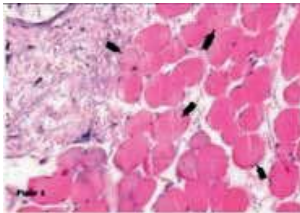

Biodegradable

Biodegradable with Full Resorption. With its optimized porous structure and chemical composition, Powerbone grafts are optimised for bone healing. During the healing process, silicate is adsorbed first followed by the β -TCP scaffold in 4 -6 months promoting replacement with native new bone.



For product dimensions and reference numbers, please refer to the product lists at the end of the catalogue.

Safe, Biocompatible and Sterile


Powerbone grafts are supplied sterile and CE marked as a Class III Medical Device according to 93/42 / EC directive. Biocompatibility (in vitro and in vivo), biodegradation, bioburden and sterility tests are applied to each material.

Radiopaque

CT and X-ray traceability is possible.




SILICATE ADDITIVE FLEXIBLE STRIP

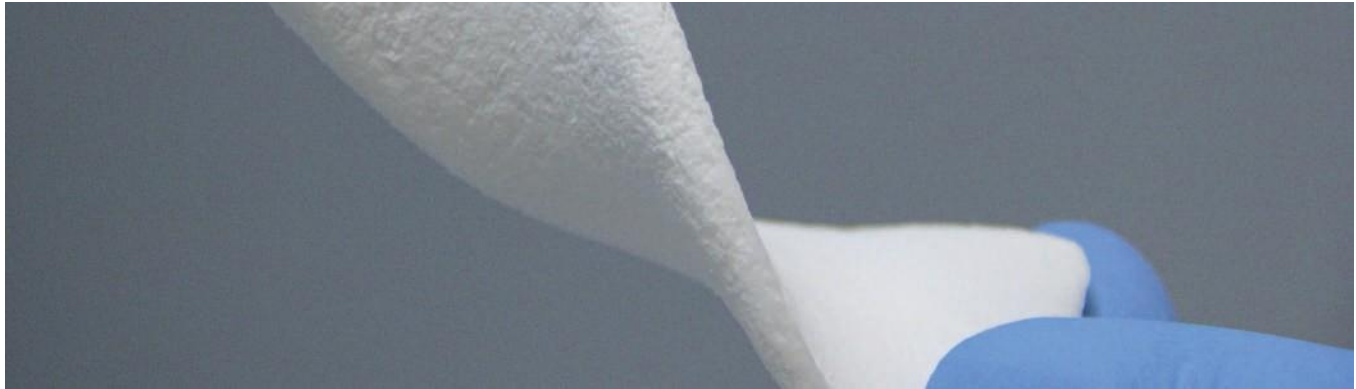

Powerbone Flexible Strip is a biodegradable synthetic bone graft that is easy to use due to its high elasticity, especially in bone defects of the pelvis and lower extremities as well as posteriolateral spinal fusion cases. Dental applications include ridge augmentation as an alternative to autogenous bone plates.

Powerbone Flexible Strip consists of silicate-added B-TCP embedded inside a PLA based synthetic polymer lattice of varying thicknesses. Osteoinductive characteristic are achieved through the addition of silicate to the embedded Powerbone graft material.

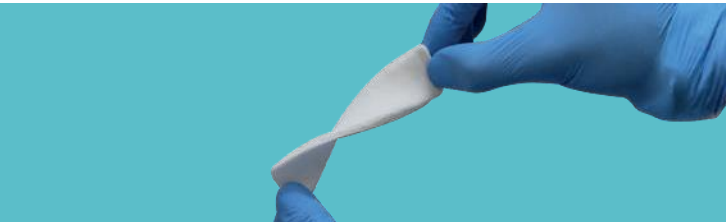

Powerbone Flexible Strip Implantation;

- Powerbone Flexible Strip can be applied to the surgical area directly or combined with bone marrow aspirate or blood.
- When wetted the flexibility of Powerbone Flexible Strip increases significantly.
- Powerbone Flexible Strip must be implanted just before all metallic implants are stabilized and the surgical site is closed.
- Powerbone Flexible Strip can be cut and placed in the spinal cage.
- Powerbone Flexible Strip gains osteoinductive characteristic due to silicate addition to the product content.


SILICATE ADDITIVE PUTTY & GEL & DENTAL PUTTY



- Minimally invasive surgical application
- Quick and easy application. Does not require mixing.
- Accelerates Bone formation.



- Designed for the healthy development of bone and periodontal support tissue.



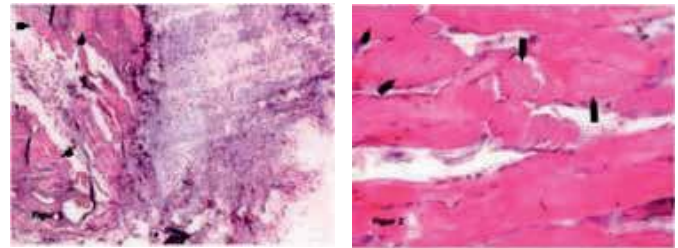


- Composed of silicate added B-TCP and resorbable cellulose carriers of varying viscosities.
- Powerbone syringe delivered grafts gains osteoinductive properties due to silicate addition.

For product dimensions and reference numbers,
please refer to the product lists at the end of the catalogue.


For product dimensions and reference numbers, please refer to the product
lists at the end of the catalogue.

UNIVERSITÄTS
KLINIKUM FREIBURG

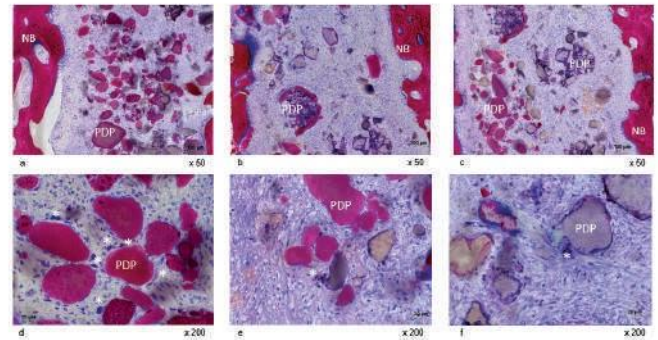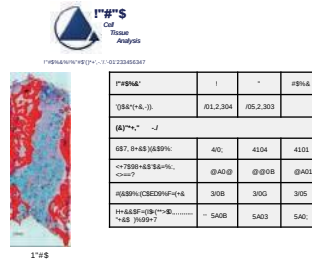

a-f) PDP surrounded by connective tissue.
b) Occasionally, Osteoid (O) detectable.
d-f) Extraordinary amount of multinucleated giant cells (MNGs, Asterisk*) visible.
d-f) PDP appears biphasic (grey and pink).

Case performed by Dr. Minas Leventis, DDS, MSc, PhD, TR

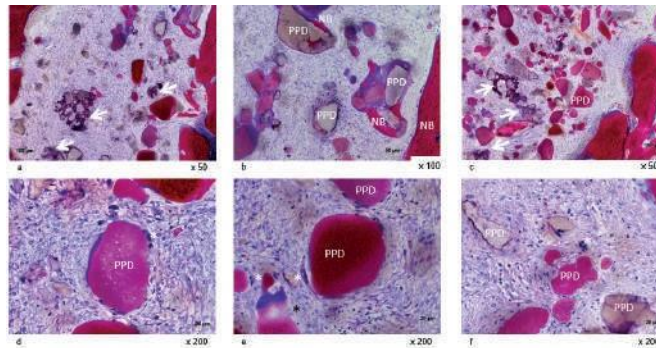

a-b) PDP surrounded by connective tissue. Plenty of multinucleated giant cells (MNGs,) visible as well as b) Many PDP particles demonstrate new bone formation (NB) at the particle surface.
a-b) PDP appears biphasic (grey and pink). Some particles seem to be in dissolution (arrow →).

DENTAL BARRIER MEMBRANE

Powerbone Barrier Membrane is:


- Designed for the healthy development of bone and periodontal support tissue.

- Composed of a poly (lactic acid) based synthetic polymer that is biocompatible and resorbable with an excellent safety profile in medical applications.


The three-layered structure of Powerbone Barrier Membrane prevents the migration of epithelial and fibroblast cells, selectively supporting the healthy development of bone and periodontal tissues. Bonegraft Barrier Membrane preserves its structure for 10-12 weeks and is completely adsorbed.

Powerbone Barrier Membrane does not contain human or animal tissue, removing any risk of viral or disease transmission as well as complying with the wishes of vegans who avoid animal derived products.

Due to its complete resorption, a second surgery for removal is not required.

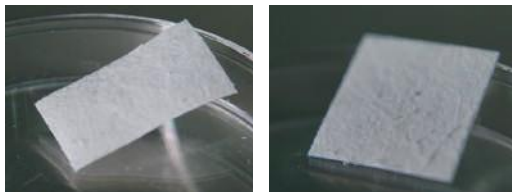

For product dimensions and reference numbers, please refer to the product lists at the end of the catalogue.

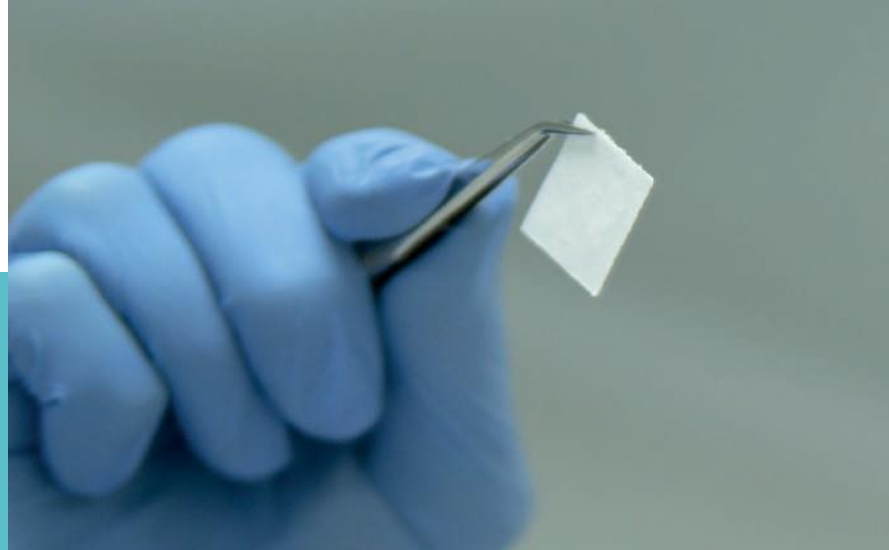


Powerbone Barrier Membrane Application

The outer surface of the Powerbone Barrier Membrane, consists of a compressed (non porous) poly (lactic acid) (PLA) layer which is placed next to the soft tissue to exclude epithelial and fibroblast cells from the site.

The inner surface of the Bonegraft Barrier Membrane faces the bony surface and consists of porous poly (lactic acid) (PLA) microfibers which induce mesenchymal stem cell retention proliferation and differentiation.

The three-layered barrier membrane is designed for the healthy development of bone and periodontal support tissue.

CHONDRO MATRIX

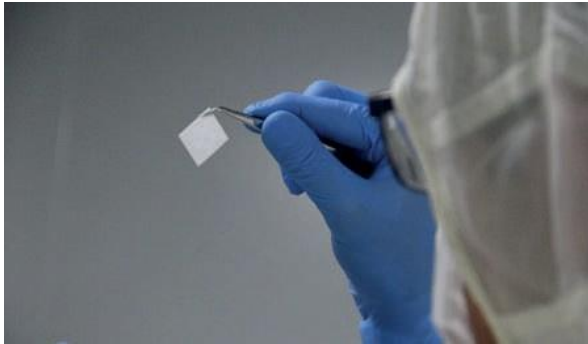

Powerbone Chondro Matrix is one-step, hydrophilic, sterile, bioresorbable, CE marked, cell-free implant used to treat articular cartilage defects in the knee, ankle or hip. It uses the biological potential of stem cells to restore damaged cartilage tissue in the joints.


Powerbone Chondro Matrix is composed of biomedical grade Polylactic acid (PLA) to provide structural support for 1-2 months and sodium hyaluronate (hyaluronic acid) to promote chondrogenesis.

Chondro Matrix does not contain human or animal tissue, removing any risk of viral or disease transmission as well as complying with the wishes of vegans who avoid animal derived products.

Due to its complete resorption, a second surgery for removal is not required.

Used for repair and surgical treatment of pain and limited mobility. When placed next to the damaged area, Chondro Matrix absorbs the accumulated blood and provides optimal defect coverage, induces the formation of cartilage repair tissue, reduces pain and symptoms associated with joint defects, and improves patients' quality of life and mobility.

For product dimensions and reference numbers, please refer to the product lists at the end of the catalogue.

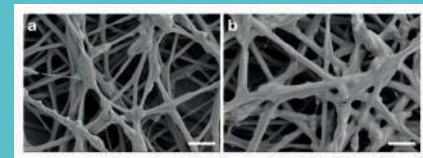

Chondro Matrixes low (a) and high (b) magnification SEM image.

Use of Bonegraft Chondro Matrix;

1 Microfracturing

- Mesenchymal stem cells are obtained by Marrow stimulating procedures, such as microfracturing or Priddle drilling.

2 Preparation and Implantation of Powerbone Chondro Matrix

- Powerbone Chondro matrix can be easily trimmed to match the defect.
- Powerbone Chondro matrix is implanted into the defective cartilage by mini-open or keyhole procedure.

3 Fixation of Powerbone Chondro Matrix





- Powerbone Chondro matrix can be fixed to the defect by commonly used orthopaedic fixation methods.
- Bioresorbable pins.
- Cartilage suture.
- Fibrin glue.

BONE CEMENT

- Polymethyl methacrylate (PMMA) based Bone Cement is a widely used biomaterial due to its ease of use in clinical practice and its long survival rate, especially with prosthetics.
- Common indications for using Bone Cement: total joint replacement, bone and joint reconstructions, fracture fixation and treatment of osteoporotic vertebral fractures.
- Bone Cement consists of two phases, solid and liquid phases.
- Powerbone Bone Cement it is presented in three different viscosities as low, standard and high.
- Dough and setting times, maximum temperature and mechanical strength values are matched to Internationally recognised ISO 5833 standards.




Compressive Strength Comparison

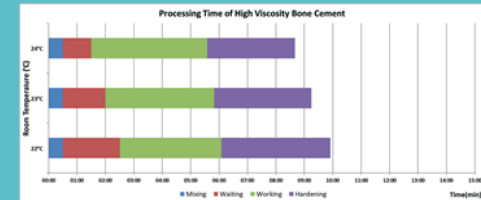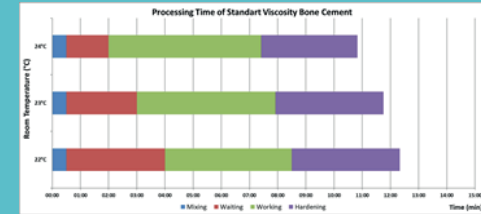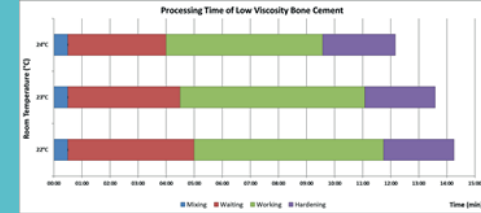


INTERFERENCE SCREW

Interference screw is a fixation device used to rigidly fix bone-patellar tendon-bone graft both in femoral and tibial tunnels and anterior cruciate ligament (ACL) reconstruction.

- Poly (L- D, Lactide) (70/30) polymer or Poly (L-D, L Lactide) (70-30)+ β -TCP (70/30) composite implants are absorbed in the body and revision surgeries are not needed.
- Used in anterior and posterior cruciate ligament surgery for temporary fixation of tendon bone and soft tissue.
- The interference screw device is supplied sterile and carries Class III Medical Device status according to the CE directive 93/42/EC. Biocompatibility, biodegradation, bioburden and sterility tests are applied to each batch to ensure predictable performance.

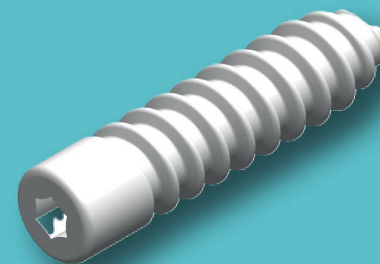

Poly (L-D, Lactide) (70/30) + β -TCP

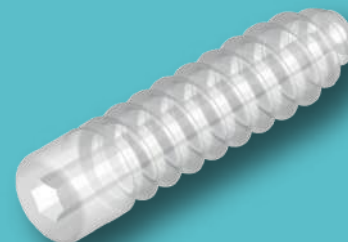


Poly (L-D Lactide) (70/30)

BIOABSORBABLE FACE LIFTING DEVICE

TRANSBLEPH

- Fast way to achieve upper periorbital region rejuvenation. This device provides versatility to combine upper eyelid skin removal with brow and upper eyelid repositioning in a single surgical session.
- Using the required upper blepharoplasty incision as an entry port, transbleph assists the surgeon in a holistic approach to the upper periorbital region. The device is easy to implement in the field and no extra hardware is required, meaning fewer tools for installation, handling and maintenance.

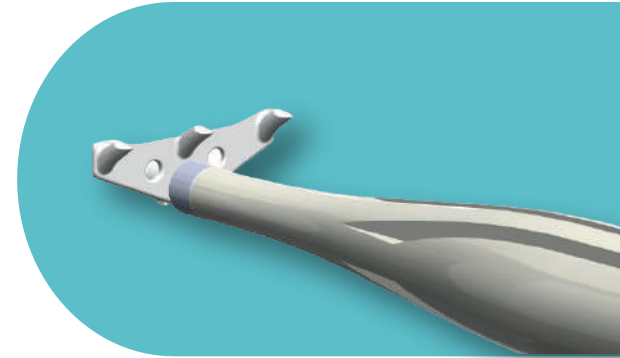

Transbleph

FOREHEAD

- Optimized size for sensitive applications forehead provides a smaller implant scale with the same predictability and safety for finer local precision applications in the forehead area. It also offers a suitable solution for patients with thicker, soft tissue and forehead skin.
- An ultra-thin platform with multiple ultra-thin spines that are unaffected by palpability but provide sensitivity for patients with all the physical characteristics of the larger Forehead scale.





Forehead

BONE SCRAPER

The Powerbone Bone Scraper is produced from a non toxic polymer. A stainless steel cutter is used to scrape and collect autogenous bone fragments from the chin or ramus area.

Powerbone Bone Scraper is designed for use by a suitable qualified clinician.

The Powerbone Bone Scraper is a disposable device used to collect autogenous bone particles for use in guided bone regeneration procedures.

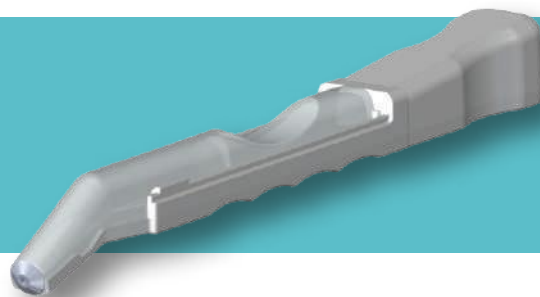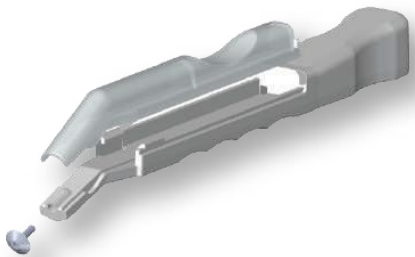

Bone Scraper Application

The resulting bone fragments provide a high volume due to their curved shape, which significantly reduces the amount of augmentation material required and reduces the invasiveness of the intervention.


Powerbone Scrapers offer the possibility of obtaining both cortical and spongy bone. Manual removal mixes bone fragments directly with patient blood and retains cellular components such as osteocytes for optimal bone regeneration.

TITANIUM PIN SET (GRADE 5)

PROPERTIES

Ergonomically designed for easy capture and quick application of titanium pins. The Bonegraft Pin Applicator offers single-handed fixation of resorbable and non-resorbable membranes.

- The ergonomic design of the applicator allows easy removal of the pin and easy fixation of the membrane. The notch, which is approximately half the length of the pin, ensures that the pin engages bone easily.
- The pin head macro geometry allows insertion without bone preparation whilst the head design prevents bending during application. These features result in higher torque insertion, better primary stability, and a more predictable success rate.
- Distortion of the pin apex during handling cannot occur.

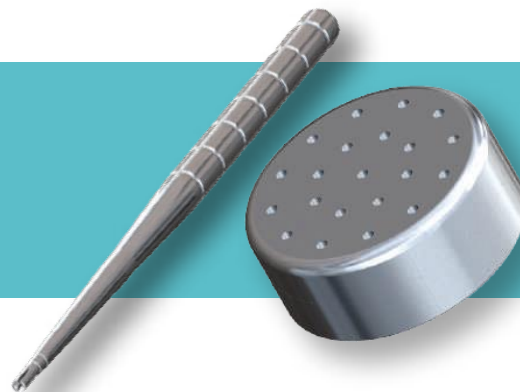

Length

- 3 mm
- 5 mm


ALLOGRAFT

- It is osteoconductive, osteoinductive and demineralised. There is a patient follow-up form in the product box. The product is processed in accordance with GMP standards. The material content is of 100% human origin. It is biocompatible with human tissue. Necessary infective tests are done.
- The shelf life of the product is 5 years and is processed who has the ISO 13485 Quality Management System Certificate obtained from the accredited institution.
- It is aseptically processed and sterilized by the Gamma irradiation method.
- Processing company is a member of European Association of Tissue Banks.




PERI-IMPLANT-RING

- Peri-Implant-Ring material consists of silicate-added β -TCP embedded inside a PLA based synthetic polymer lattice.
- The product is presented as a flexible ring structure.
- Powerbone Flexible Ring does not contain human and animal origin tissue or blood derivatives.
- It is sterilized by Gama radiation and it is osteoconductive and osteoinductive.
- The shelf life of the product is 3 years.

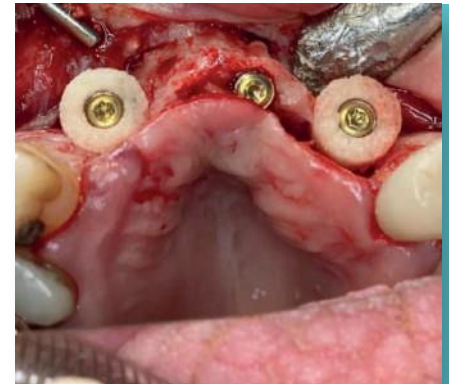

CORTICAL PLATE



- The cortical plate consists of synthetic composite materials (PLGA + β -TCP).
- Cortical Plate is used for bone fixation in trauma and reconstructive surgical operations.
- Cortical Plate is bioabsorbable and disposable.
- Cortical Plate does not contain human and animal origin tissue or blood derivatives
- Cortical Plate is MR or CT safe and is sterilized with Ethylene Oxide. Cortical Plate is biocompatible with human tissue. The shelf life of the product is 3 years. Cortical Plate carries the CE mark as a medical device and must have been produced by the manufacturer who has the ISO 13485 Quality Management System Certificate obtained from the accredited institution.

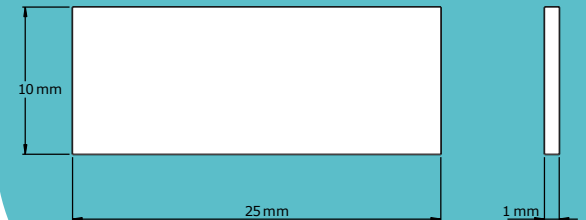

Granule (90% HA 10% β -TCP)

Osteoconductive and Osteoinductive

- Shelf life is 5 years.
- The product is produced by bonegraft who is a manufacturer the ISO 13485 Quality Management System Certificate obtained from the accredited institution.
- It is biocompatible with human tissue
- It is osteoconductive and osteoinductive.
- It must be sterilized by the Gamma irradiation method.
- The product is similar structure to the mineral present in the bone.



- Its optimized porous structure and chemical composition, it should be suitable for the continuous regeneration cycle of bone.
- While the granule containing only β -TCP degrades in 6-12 months during the healing process, in the combination of 90% HA and 10% β -TCP, β -TCP degrades first and then HA, this process takes 12-18 months and supports bone formation.





The combination of 90% HA and 10% β -TCP allows the degradation kinetics to be adjusted in vitro and in vivo. Elicits similar responses to in vitro and in vivo responses by bone and promotes cell attachment, proliferation, and expression. The combination of 90% HA and 10% β -TCP has been successfully used in many clinical situations such as repair of bone defects, bone augmentation in spinal arthrodesis, periodontal treatment, or coating for metallic implants.

FIXATION SCREW (GRADE 5)

Indicated for use in Guided Bone Regeneration, fixation of membranes, flexible strips, cortical grafts and meshes.

- **High stability**
The titanium alloy (grade 5) fixation screw provides high stability and there is no weakening of the material thanks to the aggressive structure of the screw.
- **Biocompatible**
The screw material helps to reduce the risk of infection and helps to prevent allergic reactions.

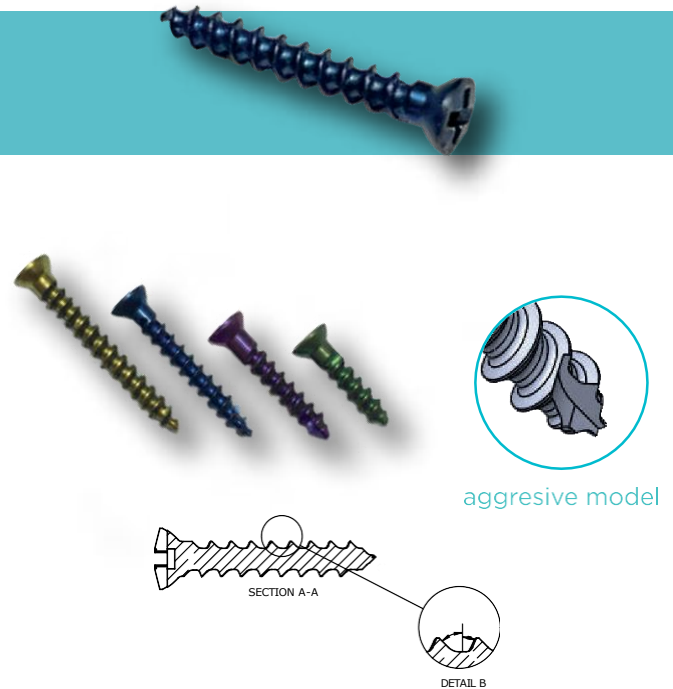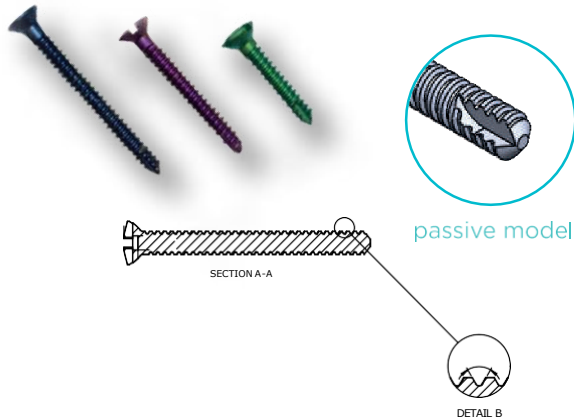

POWERBRIGHT (Home Use)

Powerbright (Home Use) is a cosmetic product designed for use in the oral cavity as a tooth whitening agent. The controlled application of the supplied agent lightens the teeth by gentle bleaching of organic pigments within the enamel.

Contents

- 8x1g teeth whitening agents.
Whitening tray.
- Contents: hydrogen peroxide, glycerol, sodium hydroxide, potassium nitrate, carbomer, aroma.
- Powerbright (Home Use) is for at-home application following the advice of a professional.



POWERBRIGHT PLUS (Office Use)

Powerbright Plus is an oral care cosmetic product used under the supervision of a professional for in office tooth whitening. Powerbright Plus lightens teeth by removing stains created by organic pigments deep in the dentin tissue.

Contents

- 0.5 g teeth whitening agents 2x1g gingival barrier.
- 2 connectors 2 syringe tips Buccal retractor
- Ingredients: hydrogen peroxide, glycerol, sodium hydroxide, potassium nitrate, carbomer Powerbright Plus is a dental agent for office use.



PRODUCT REFERENCE AND SIZES

PRODUCT REFERENCE AND SIZES

Powerbone Stick & Block & Plug



Reference Code	Size	Volume	Reference Code	Size	Volume
PS44201	4x4x20 mm(1 pcs)	2,03 cc	PS91214	9x12x14 mm	14,24 cc
PS44202	4x4x20 mm(2 pcs)	4,05 cc	PS91216	9x12x16 mm	16,27 cc
PS44206	4x4x20 mm(6 pcs)	12,15 cc	PS101147	10x11x47 mm	10,00 cc
PS55204	5x5x20 mm(4 pcs)	16,50 cc	PS111947	11x19x47 mm	20,00 cc
PS55205	5x5x20 mm(5 pcs)	20,63 cc	PS1010402	10x10x40 mm(2 pcs)	19,90 cc
PS55206	5x5x20 mm(6 pcs)	24,76 cc	PSC5204	5x20 mm	12,96 cc
PS5510	5x5x10 mm	2,06 cc	PSC6204	6x20 mm	15,56 cc
PS5520	5x5x20 mm	4,13 cc	PSC8204	8x20 mm	20,76 cc
PS5617	5x6x17 mm	4,21 cc	PW062530	6x25x30mm	5,15 cc
PS5634	5x6x34 mm	8,42 cc	PW082530	8x25x30 mm	7,65 cc
PS6717	6x7x17 mm	5,89 cc	PW102530	10x25x30 mm	10,15 cc
PS6734	6x7x34 mm	11,78 cc	PW122530	12x25x30 mm	15,15 cc
PS8820	8x8x20 mm	10,56 cc	PW142530	14x25x30 mm	20,15 cc
PS101020	10x10x20 mm	16,50 cc	PW061520	6x15x20 mm	2,06 cc
PS151520	15x15x20 mm	24,50 cc	PW081520	8x15x20 mm	2,75 cc
PS71214	7x12x14 mm	9,69 cc	PW101520	10x15x20 mm	3,44 cc
PS71216	7x12x16 mm	11,07 cc	PW121520	12x15x20mm	4,13 cc
PS81214	8x12x14 mm	11,07 cc	PW141520	14x15x20 mm	4,82 cc
PS81216	8x12x16 mm	12,66 cc			

PRODUCT REFERENCE AND SIZES

Powerbone Granule



Powerbone Granule in the Bottle



Reference Code	Size	Volume	Reference Code	Size	Volume
PG02501005	0.25-1 mm	0,5 cc	PG020415	2-4 mm	15 cc
PG02501010	0.25-1 mm	1 cc	PG020420	2-4 mm	20 cc
PG02501020	0.25-1 mm	2 cc	PG020430	2-4 mm	30 cc
PG05001005	0.5-1 mm	0,5 cc	PG030505	3-5 mm	5 cc
PG05001010	0.5-1 mm	1 cc	PG030510	3-5 mm	10 cc
PG05001020	0.5-1 mm	2 cc	PG030515	3-5 mm	15 cc
PG05001050	0.5-1 mm	5 cc	PG030520	3-5 mm	20 cc
PG05001075	0.5-1 mm	7,5 cc	PG0305230	3-5 mm	30 cc
PG05001100	0.5-1 mm	10 cc	PG040705	4-7 mm	5 cc
PG10002005	1-2 mm	0,5 cc	PG0407075	4-7 mm	7,5 cc
PG10002010	1-2 mm	1 cc	PG040710	4-7 mm	10 cc
PG10002020	1-2 mm	2 cc	PG040715	4-7 mm	15 cc
PG10002050	1-2 mm	5 cc	PG040720	4-7 mm	20 cc
PG10002075	1-2 mm	7,5 cc	PG040730	4-7 mm	30 cc
PG10002100	1-2 mm	10 cc	PG070905	7-9 mm	5 cc
PG10002150	1-2 mm	15 cc	PG0709075	7-9 mm	7,5 cc
PG10002200	1-2 mm	20 cc	PG070910	7-9 mm	10 cc
PG10002300	1-2 mm	30 cc	PG070915	7-9 mm	15 cc
PG020405	2-4 mm	5 cc	PG070920	7-9 mm	20 cc
PG0204075	2-4 mm	7,5 cc	PG070930	7-9 mm	30 cc
PG020410	2-4 mm	10 cc			

Reference Code	Size	Volume	Reference Code	Size	Volume
PCSGB02501005	0.25-1 mm	0,5 cc	PCSGB10002005	1-2 mm	0,5 cc
PCSGB02501010	0.25-1 mm	1 cc	PCSGB10002010	1-2 mm	1 cc
PCSGB02501020	0.25-1 mm	2 cc	PCSGB10002020	1-2 mm	2 cc
PCSGB05001005	0.5-1 mm	0,5 cc	PCSGB10002050	1-2 mm	5 cc
PCSGB05001010	0.5-1 mm	1 cc	PCSGB10002100	1-2 mm	10 cc
PCSGB05001020	0.5-1 mm	2 cc			
PCSGB05001050	0.5-1 mm	5 cc			
PCSGB05001100	0.5-1 mm	10 cc			

PRODUCT REFERENCE AND SIZES

Powerbone Putty



Reference Code	Volume
PP005	0,5 cc
PP006	0,6 cc
PP01	1 cc
PP02	2 cc
PP03	3 cc
PP05	5 cc
PP06	6 cc
PP075	7,5 cc
PP10	10 cc

Powerbone Flex



Powerbone Gel



Reference Code	Volume
PG01	1 cc
PG02	2 cc
PG03	3 cc
PG05	5 cc
PG06	6 cc
PG10	10 cc

Powerbone Dental Putty



Reference Code	Volume
PDP030	0,3 cc
PDP050	0,5 cc
PDP075	0,75 cc
PDP100	1 cc

Reference Code	Size	Volume
PFS25254	25x25x4mm	2,50 cc
PFS25504	25x50x4mm	5,00 cc
PFS25505	25x50x5mm	6,25 cc
PFS50504	50x50x4mm	10,00 cc
PFS201005	20x100x5mm	10,00 cc
PFS201006	20x100x6mm	12,00 cc
PFS25754	25x75x4mm	7,50 cc
PFS25804	25x80x4mm	8,00 cc
PFS25805	25x80x5mm	10,00 cc
PFS60606	60x60x6mm	21,60 cc
PFS35605	35x60x5mm	10,50 cc
PFS75405	75x40x5mm	15,00 cc
PFS25252	25x25x2mm	2,50 cc
PFS25502	25x50x2mm	5,00 cc
PFS25802	25x80x2mm	8,00 cc
PFS35602	35x60x2mm	10,50 cc
PFS60602	60x60x2mm	21,60 cc

PRODUCT REFERENCE AND SIZES

Powerbone Barrier Membrane



Reference Code	Size
PM1520	15X20 mm
PM1525	15x25 mm
PM2020	20x20 mm
PM2025	20x25 mm
PM2030	20x30 mm
PM2530	25x30 mm
PM3040	30x40 mm
PM1520-5	15x20 mm(5pcs)
PM1525-5	15x25 mm(5pcs)
PM2020-5	20x20 mm(5pcs)
PM2030-5	20x30 mm(5pcs)

Powerbone Chondro Matrix



Reference Code	Size
PK202011	20-20-1,1 mm
PK203011	20-30-1,1 mm
PK251711	25-17-1,1 mm
PK252511	25-25-1,1 mm
PK253511	25-35-1,1 mm
PK353511	35-35-1,1 mm

Powerbone Bone Cement



Reference Code	Size
PVC-LV-20	20 g (LV Radiopaque Vertebroplasty Bone Cement)
PVC-LV-40	40 g (LV Radiopaque Vertebroplasty Bone Cement)
PKC-LV-20	20 g (LV Radiopaque Kyphoplasty Bone Cement)
PKC-LV-40	40 g (LV Radiopaque Kyphoplasty Bone Cement)
POC-SV40	40 g (Radiopaque Bone Cement Normal for ortho)
P-PC-HV	40 g (Radiopaque Bone Cement-HV for ortho)

PRODUCT REFERENCE AND SIZES

Powerbone PLDLLA-TCP 30 Interference Screws



Reference Code	Size
SCRW-PPT30IS720	7mm x 20mm
SCRW-PPT30IS725	7mm x 25mm
SCRW-PPT30IS730	7mm x 30mm
SCRW-PPT30IS820	8mm x 20mm
SCRW-PPT30IS825	8mm x 25mm
SCRW-PPT30IS830	8mm x 30mm
SCRW-PPT30IS835	8mm x 35mm
SCRW-PPT30IS920	9mm x 20mm
SCRW-PPT30IS925	9mm x 25mm
SCRW-PPT30IS930	9mm x 30mm
SCRW-PPT30IS935	9mm x 35mm
SCRW-PPT30IS1025	10mm x 25mm
SCRW-PPT30IS1030	10mm x 30mm
SCRW-PPT30IS1025	10mm x 25mm
SCRW-PPT30IS1030	10mm x 30mm
SCRW-PPT30IS1035	10mm x 35mm
SCRW-PPT30IS1135	10mm x 35mm

Powerbone PLA Interference Screws



Reference Code	Size
SCRW-PPIS720	7mm x 20mm
SCRW-PPIS725	7mm x 25mm
SCRW-PPIS730	7mm x 30mm
SCRW-PPIS820	8mm x 20mm
SCRW-PPIS825	8mm x 25mm
SCRW-PPIS830	8mm x 30mm
SCRW-PPIS920	9mm x 20mm
SCRW-PPIS925	9mm x 25mm
SCRW-PPIS930	9mm x 30mm
SCRW-PPIS1020	10mm x 20mm
SCRW-PPIS1025	10mm x 25mm
SCRW-PPIS1030	10mm x 30mm

PRODUCT REFERENCE AND SIZES

Powerbone TRANSBLEPH Device



Reference Code

C-EST-PTD30
C-EST-PTD35

Size

3,0 mm (height of pins)
3,5 mm (height of pins)

Powerbone FOREHEAD Lift Device



Reference Code


C-EST-PFLD30
C-EST-PFLD35

Size

3,0 mm (height of pins)
3,5 mm (height of pins)

PRODUCT REFERENCE AND SIZES

Bone Scraper

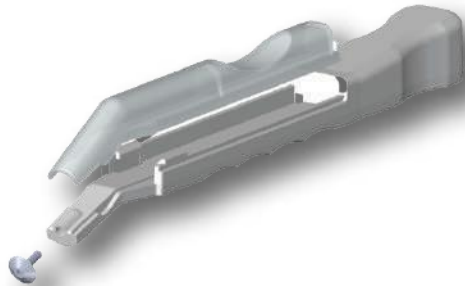

Reference Code

PBS

Size

1.48cm x 16cm (1pc)

Titanium Pin Set (Grade5)



Reference Code

Power-398.0002530

Power-398.0002550

Size

2.5x3,00mm

2.5x5,00mm

PRODUCT REFERENCE AND SIZES

ALLOGRAFT




Reference Code	Size	Volume
PWB2024FD	0.25-1 mm	0,5 cc
PWB2025FD	0.25-1 mm	1 cc
PWB2027FD	0.25-1 mm	2 cc
PWB2028FD	0.25-1 mm	5 cc

PERI IMPLANT RING



Reference Code	Size
PFSC320	3x20 mm
PFSC620	6x20 mm

CORTICAL PLATE

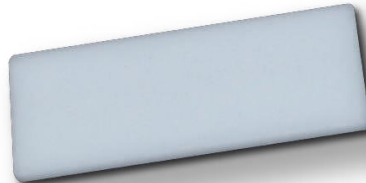

Reference Code	Size
C-PLT-B219HPS115	25x10x1 mm

PRODUCT REFERENCE AND SIZES

Powerbone Granule
(90% HA 10% β -TCP)



Reference Code	Size	Volume
PGB05001005HA	0.5-1 mm	0,5 cc
PGB05001010HA	0.5-1 mm	1cc
PGB05001020HA	0.5-1 mm	2 cc
PGB05001050HA	0.5-1 mm	5 cc
PGB05001150HA	0.5-1 mm	15 cc

PRODUCT REFERENCE AND SIZES



aggressive model

Reference Code	Size
Power-TPSS	6,80 mm
Power-TPSL	8,80 mm
Power-TPSM	10,80 mm
Power-TPSK	12,80 mm



passive model

Reference Code	Size
Power-TPSS	7 mm
Power-TPSL	10 mm
Power-TPSM	13 mm

PRODUCT REFERENCE AND SIZES

(Home Use)
POWERBRIGHT
%6 HP



Reference Code

PWA06-01

(Office Use)
POWERBRIGHT PLUS
%35 HP



Reference Code

PPWA35-01

The logo for Rebound Global Trading Co. features the word "rebound" in a blue, lowercase, sans-serif font. The letter "o" is replaced by a blue circle containing a white globe icon. A green checkmark is positioned behind the "o" and extends upwards and to the right. Below "rebound" is the text "GLOBAL TRADING CO." in a bold, black, uppercase, sans-serif font.

rebound

GLOBAL TRADING CO.

Cevizli Mah. Zuhal Cad.. Ritim İstanbul Sit. A5 Blk. No :46E/179 MALTEPE
İSTANBUL
0 542 387 01 27
0 530 328 12 61
info@reboundtr.com